

seleXys (excluding seleXys PC) Total Conventional Hip Investigation

Note: This analysis compares the seleXys (excluding seleXys PC) acetabular prosthesis with all other total conventional hip prostheses.

This prosthesis has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2024>.

Note: Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator. Procedures using prostheses with no recorded use in 2023 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Conventional Hip Replacement

The revision rate of the seleXys (excluding seleXys PC) total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 1: Revision Rates of Primary Total Conventional Hip Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
seleXys (excluding seleXys PC)	52	391	3884	1.34 (1.00, 1.76)
Other Total Conventional Hip	19221	538380	3453178	0.56 (0.55, 0.56)
TOTAL	19273	538771	3457063	0.56 (0.55, 0.57)

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the seleXys (excluding seleXys PC) total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 2: Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs
seleXys (excluding seleXys PC)	4.6 (2.9, 7.2)	6.7 (4.6, 9.7)	7.8 (5.5, 11.0)	9.7 (7.1, 13.2)	10.6 (7.9, 14.1)	11.1 (8.3, 14.8)	12.3 (9.4, 16.1)	12.6 (9.6, 16.5)
Other Total Conventional Hip	1.7 (1.7, 1.8)	2.2 (2.1, 2.2)	2.5 (2.5, 2.5)	2.8 (2.7, 2.8)	3.1 (3.0, 3.1)	3.3 (3.3, 3.4)	3.6 (3.6, 3.7)	3.9 (3.8, 4.0)

CPR	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs
seleXys (excluding seleXys PC)	13.0 (9.9, 16.8)	13.3 (10.2, 17.2)	13.3 (10.2, 17.2)	13.7 (10.6, 17.8)	13.7 (10.6, 17.8)	13.7 (10.6, 17.8)	17.1 (12.1, 23.7)	
Other Total Conventional Hip	4.2 (4.1, 4.3)	4.5 (4.5, 4.6)	4.9 (4.8, 4.9)	5.3 (5.2, 5.4)	5.7 (5.6, 5.8)	6.0 (5.9, 6.2)	6.5 (6.3, 6.6)	6.9 (6.7, 7.0)

CPR	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
seleXys (excluding seleXys PC)							
Other Total Conventional Hip	7.3 (7.1, 7.4)	7.6 (7.5, 7.8)	8.2 (8.0, 8.4)	8.5 (8.2, 8.7)	9.0 (8.7, 9.3)	9.7 (9.2, 10.1)	10.3 (9.5, 11.2)

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.


FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the seleXys (excluding seleXys PC) total conventional hip prosthesis is compared to all other total conventional hip prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Conventional Hip Replacement

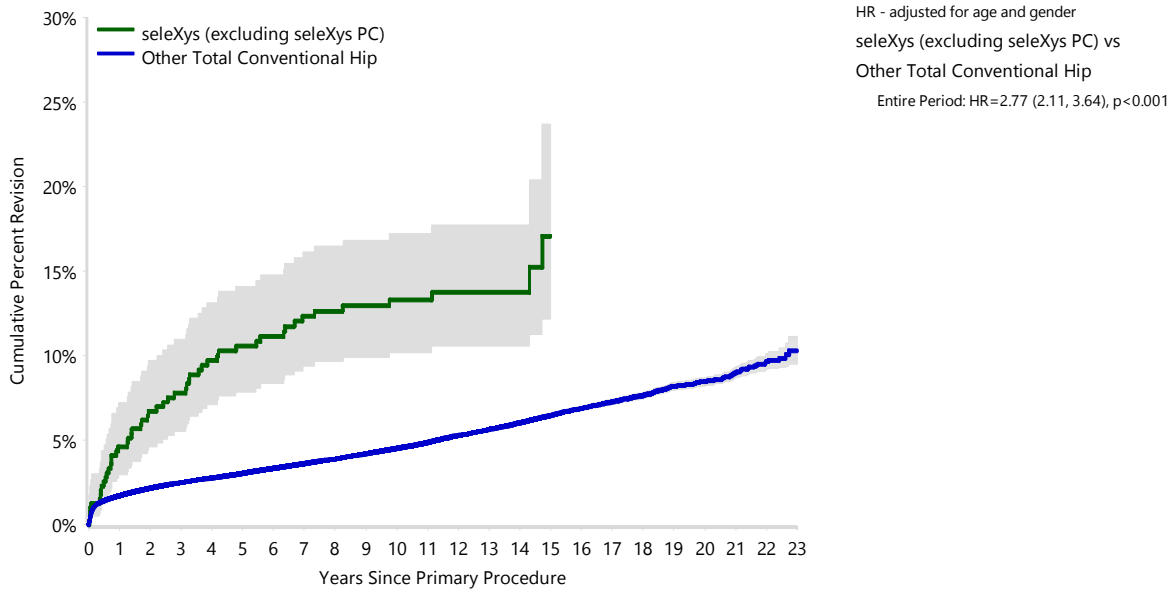

Number at Risk	0 Yr	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs
seleXys (excluding seleXys PC)	391	369	353	341	325	314	302	288	278	270	256	204
Other Total Conventional Hip	538380	475497	425667	377035	332783	288854	247665	209507	174463	143193	117723	96178

Number at Risk	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
seleXys (excluding seleXys PC)	146	99	63	43	31	12	0	0	0	0	0	0
Other Total Conventional Hip	77763	61577	47693	35979	26857	20094	14821	10048	6170	3221	1205	203

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 3**Primary Diagnosis for Revised Primary Total Conventional Hip Replacement**

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total conventional hip prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Conventional Hip Replacement

Primary Diagnosis	seleXys (excluding seleXys PC)		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Osteoarthritis	49	94.2	15924	82.8
Fractured Neck Of Femur	1	1.9	1420	7.4
Osteonecrosis	2	3.8	858	4.5
Developmental Dysplasia			320	1.7
Rheumatoid Arthritis			208	1.1
Failed Internal Fixation			151	0.8
Tumour			149	0.8
Other Inflammatory Arthritis			106	0.6
Fracture/Dislocation			53	0.3
Other			17	0.1
Arthrodesis Takedown			15	0.1
TOTAL	52	100.0	19221	100.0

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Conventional Hip Replacement - Reason for Revision (Follow-up Limited to 17.8 Years)

Revision Diagnosis	seleXys (excluding seleXys PC)			Other Total Conventional Hip		
	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	2	0.5	3.8	4488	0.8	23.5
Prosthesis Dislocation/Instability	5	1.3	9.6	4364	0.8	22.9
Fracture	4	1.0	7.7	4237	0.8	22.2
Loosening	31	7.9	59.6	3765	0.7	19.7
Pain	1	0.3	1.9	334	0.1	1.8
Leg Length Discrepancy				291	0.1	1.5
Malposition	3	0.8	5.8	264	0.0	1.4
Lysis	1	0.3	1.9	201	0.0	1.1
Implant Breakage Stem	1	0.3	1.9	188	0.0	1.0
Implant Breakage Acetabular Insert				130	0.0	0.7
Incorrect Sizing	1	0.3	1.9	103	0.0	0.5
Wear Acetabular Insert	1	0.3	1.9	102	0.0	0.5
Metal Related Pathology	1	0.3	1.9	78	0.0	0.4
Implant Breakage Acetabular				71	0.0	0.4
Wear Head				46	0.0	0.2
Tumour				44	0.0	0.2
Implant Breakage Head				32	0.0	0.2
Heterotopic Bone				26	0.0	0.1
Wear Acetabulum				10	0.0	0.1
Osteonecrosis				2	0.0	0.0
Progression Of Disease				2	0.0	0.0
Synovitis				1	0.0	0.0
Other	1	0.3	1.9	291	0.1	1.5
N Revision	52	13.3	100.0	19070	3.5	100.0
N Primary	391			538380		

Note: This table is restricted to revisions within 17.8 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Conventional Hip Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the seleXys (excluding seleXys PC) total conventional hip prosthesis. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total conventional hip prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Conventional Hip Replacement

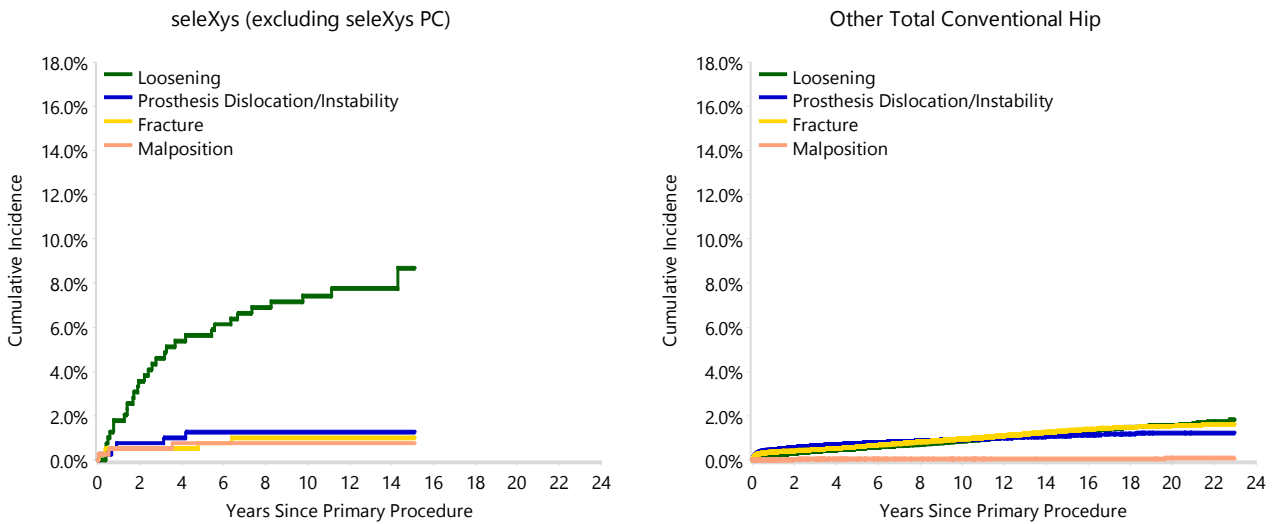


TABLE 5

Type of Revision Performed for Primary Total Conventional Hip Replacement

This analysis identifies the components used in the revision of the seleXys (excluding seleXys PC) total conventional hip prosthesis and compares it to the components used in the revision of all other total conventional hip prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total conventional hip prostheses i.e. is there a difference in the type of revision undertaken for the seleXys (excluding seleXys PC) total conventional hip prosthesis compared to all other total conventional hip prostheses.

Table 5: Primary Total Conventional Hip Replacement - Type of Revision (Follow-up Limited to 17.8 Years)

Type of Revision	seleXys (excluding seleXys PC)		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Femoral Component	10	19.2	6313	33.1
Acetabular Component	32	61.5	3541	18.6
THR (Femoral/Acetabular)	4	7.7	2218	11.6
Cement Spacer	2	3.8	620	3.3
Removal of Prostheses			99	0.5
Reinsertion of Components			28	0.1
Total Femoral			9	0.0
Bipolar Head and Femoral			7	0.0
Saddle			1	0.0
N Major	48	92.3	12836	67.3
Head/Insert	2	3.8	4809	25.2
Head Only	1	1.9	925	4.9
Minor Components	1	1.9	310	1.6
Insert Only			186	1.0
Bipolar Only			2	0.0
Cement Only			1	0.0
Head/Neck			1	0.0
N Minor	4	7.7	6234	32.7
TOTAL	52	100.0	19070	100.0

Note: This table is restricted to revisions within 17.8 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 6**Revision Rates of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Fixation

Fixation	N Revised	N Total
Cementless	46	348
Hybrid (Femur Cemented)	6	43
TOTAL	52	391

TABLE 7**Revision Rates of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this prosthesis are listed.

Table 7: Revised Number of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Ceramic/Ceramic	5	89
Ceramic/Non XLPE	13	64
Ceramic/XLPE + Antioxidant	22	109
Metal/Metal	1	13
Metal/Non XLPE	5	41
Metal/XLPE + Antioxidant	6	74
Ceramicised Metal/XLPE + Antioxidant	0	1
TOTAL	52	391

TABLE 8

Revision Rates of Primary Total Conventional Hip Replacement by State

This enables a state by state variation to be identified for the seleXys (excluding seleXys PC) total conventional hip prosthesis and provides the comparative data for each of the states for all other total conventional hip prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 8: Revised Number of Primary Total Conventional Hip Replacement by State

Component	State	N Revised	N Total
seleXys (excluding seleXys PC)	NSW	2	32
	VIC	33	174
	QLD	10	119
	WA	7	66
Other Total Conventional Hip	NSW	5207	157703
	VIC	4835	140581
	QLD	3787	94527
	WA	2546	63263
	SA	1825	49398
	TAS	452	18198
	ACT/NT	569	14710
TOTAL		19273	538771

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 9**Number of Revisions of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the seleXys (excluding seleXys PC) total conventional hip prosthesis. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2023 has a maximum of one year to be revised, whereas a primary procedure performed in 2021 has a maximum of three years to be revised.

Table 9: Number of Revisions of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2006	3	35
2007	4	33
2008	4	20
2009	0	21
2010	10	53
2011	12	70
2012	12	89
2013	7	57
2014	0	13
TOTAL	52	391

TABLE 10

Revision Rates of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular seleXys (excluding seleXys PC) prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Material
Acetabular				
seleXys	55400042-55400068	SELEXYS TPS SHELL	NO	METAL
seleXys	55420042-55420064	SELEXYS TH SHELL	NO	METAL
seleXys	55420142-55420164	SELEXYS TH+ SHELL	NO	METAL

Table 10: Revised Number of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Catalogue Number Range

Acetabular Range	N Revised	N Total
55400042-55400068	22	245
55420042-55420064	4	28
55420142-55420164	26	118
TOTAL	52	391

TABLE 11

Revision Rates of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Component

A prosthesis may be combined with multiple components. This analysis has been undertaken to determine if the revision rate varies according to the component with which it is combined.

Table 11: Revised Number of seleXys (excluding seleXys PC) Primary Total Conventional Hip Replacement by Femoral Stem Component

Femoral Stem Component	N Revised	N Total
Alloclassic	0	2
CBC Stem	3	16
CBH Stem	13	105
Fullfix	2	27
MS 30	1	1
SL-Plus	12	48
twinSys (cless)	18	178
twinSys (ctd)	3	14
TOTAL	52	391