

Avenir/Fitmore Total Conventional Hip Investigation

Note: This analysis compares the Avenir/Fitmore femoral stem/acetabular combination with all other total conventional hip prostheses.

This combination has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2024>.

Note: Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator. Procedures using prostheses with no recorded use in 2023 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Conventional Hip Replacement

The revision rate of the Avenir/Fitmore total conventional hip combination is compared to all other total conventional hip prostheses.

Table 1: Revision Rates of Primary Total Conventional Hip Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
Avenir/Fitmore	21	372	1443	1.46 (0.90, 2.22)
Other Total Conventional Hip	19228	538169	3453198	0.56 (0.55, 0.56)
TOTAL	19249	538541	3454641	0.56 (0.55, 0.57)

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the Avenir/Fitmore total conventional hip combination is compared to all other total conventional hip prostheses.

Table 2: Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs
Avenir/Fitmore	5.1 (3.3, 7.9)	5.5 (3.6, 8.3)	5.5 (3.6, 8.3)	5.9 (3.9, 9.0)	5.9 (3.9, 9.0)	5.9 (3.9, 9.0)	5.9 (3.9, 9.0)	
Other Total Conventional Hip	1.7 (1.7, 1.8)	2.2 (2.1, 2.2)	2.5 (2.5, 2.5)	2.8 (2.7, 2.8)	3.1 (3.0, 3.1)	3.3 (3.3, 3.4)	3.6 (3.6, 3.7)	3.9 (3.8, 4.0)

CPR	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs
Avenir/Fitmore								
Other Total Conventional Hip	4.2 (4.2, 4.3)	4.5 (4.5, 4.6)	4.9 (4.8, 5.0)	5.3 (5.2, 5.4)	5.7 (5.6, 5.8)	6.0 (5.9, 6.2)	6.5 (6.3, 6.6)	6.9 (6.7, 7.0)

CPR	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
Avenir/Fitmore							
Other Total Conventional Hip	7.3 (7.1, 7.4)	7.6 (7.5, 7.8)	8.2 (8.0, 8.4)	8.5 (8.2, 8.7)	9.0 (8.7, 9.3)	9.7 (9.2, 10.1)	10.3 (9.5, 11.2)

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.


FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the Avenir/Fitmore total conventional hip combination is compared to all other total conventional hip prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Conventional Hip Replacement

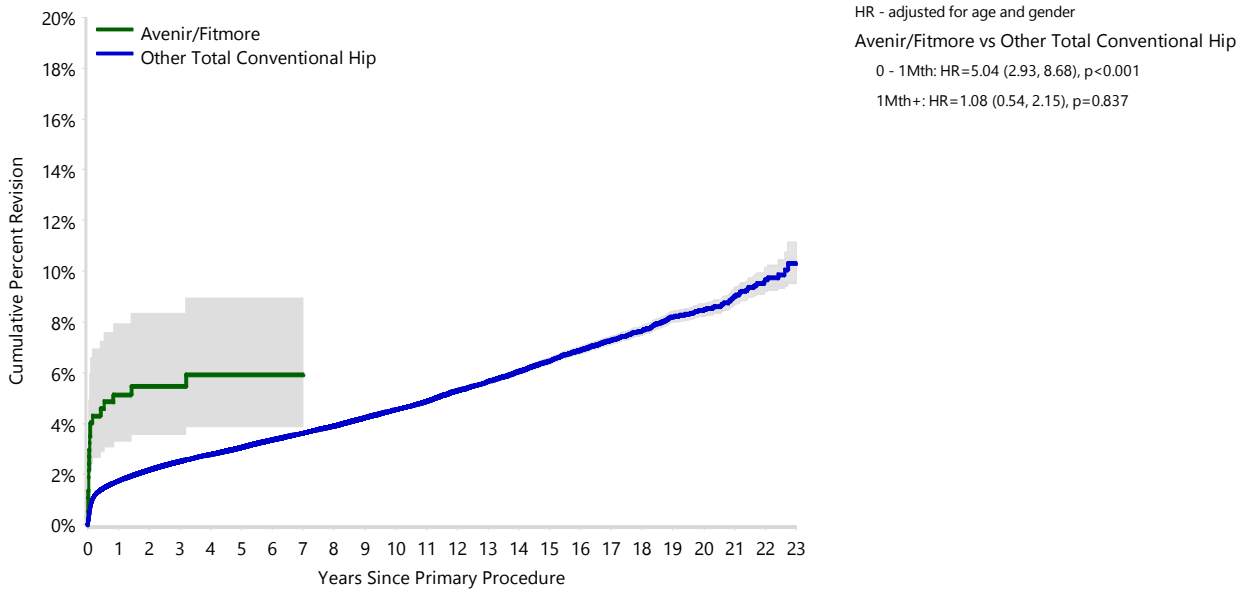

Number at Risk	0 Yr	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs
Avenir/Fitmore	372	321	279	221	179	123	86	47	9	5	2	0
Other Total Conventional Hip	538169	475324	425527	376947	332732	288856	247703	209574	174565	143296	117823	96251

Number at Risk	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
Avenir/Fitmore	0	0	0	0	0	0	0	0	0	0	0	0
Other Total Conventional Hip	77815	61602	47695	35979	26857	20094	14821	10048	6170	3221	1205	203

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 3**Primary Diagnosis for Revised Primary Total Conventional Hip Replacement**

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total conventional hip prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Conventional Hip Replacement

Primary Diagnosis	Avenir/Fitmore		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Osteoarthritis	21	100.0	15930	82.8
Fractured Neck Of Femur			1420	7.4
Osteonecrosis			859	4.5
Developmental Dysplasia			320	1.7
Rheumatoid Arthritis			208	1.1
Failed Internal Fixation			151	0.8
Tumour			149	0.8
Other Inflammatory Arthritis			106	0.6
Fracture/Dislocation			53	0.3
Other			17	0.1
Arthrodesis Takedown			15	0.1
TOTAL	21	100.0	19228	100.0

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Conventional Hip Replacement - Reason for Revision (Follow-up Limited to 10.3 Years)

Revision Diagnosis	Avenir/Fitmore			Other Total Conventional Hip		
	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	8	2.2	38.1	4315	0.8	24.7
Prosthesis Dislocation/Instability	1	0.3	4.8	4144	0.8	23.8
Fracture	5	1.3	23.8	3771	0.7	21.6
Loosening	4	1.1	19.0	3269	0.6	18.7
Pain	1	0.3	4.8	316	0.1	1.8
Leg Length Discrepancy				290	0.1	1.7
Malposition				259	0.0	1.5
Implant Breakage Stem				147	0.0	0.8
Lysis				119	0.0	0.7
Implant Breakage Acetabular Insert				112	0.0	0.6
Incorrect Sizing				102	0.0	0.6
Implant Breakage Acetabular				62	0.0	0.4
Metal Related Pathology				62	0.0	0.4
Wear Acetabular Insert				55	0.0	0.3
Tumour				42	0.0	0.2
Wear Head				40	0.0	0.2
Heterotopic Bone				26	0.0	0.1
Implant Breakage Head				26	0.0	0.1
Wear Acetabulum				6	0.0	0.0
Osteonecrosis				2	0.0	0.0
Progression Of Disease				2	0.0	0.0
Synovitis				1	0.0	0.0
Other	2	0.5	9.5	277	0.1	1.6
N Revision	21	5.6	100.0	17445	3.2	100.0
N Primary	372			538169		

Note: This table is restricted to revisions within 10.3 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Conventional Hip Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the Avenir/Fitmore total conventional hip combination. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total conventional hip prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Conventional Hip Replacement

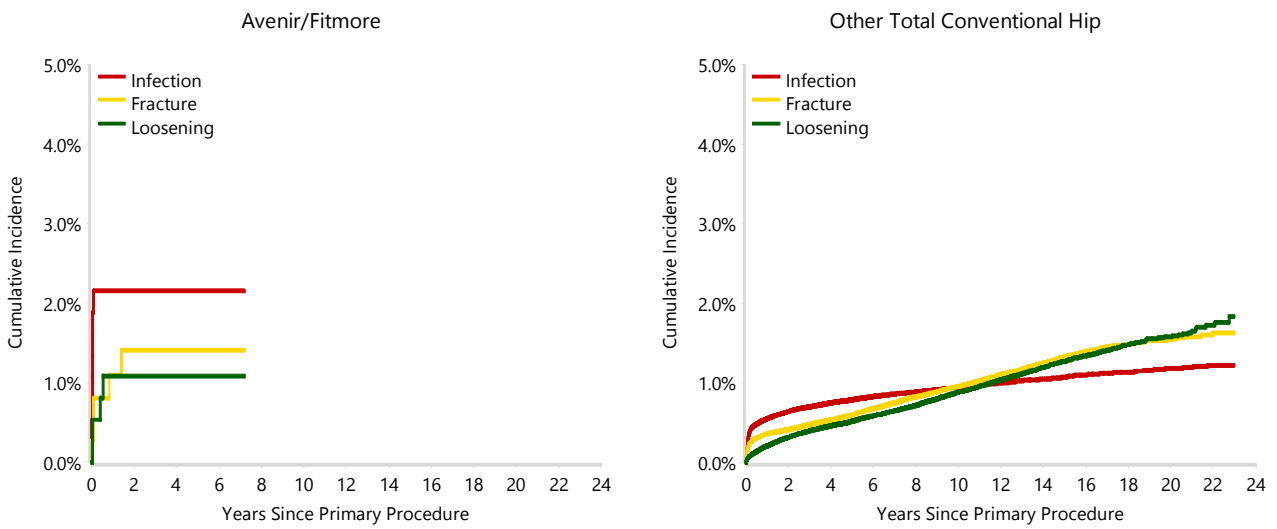


TABLE 5

Type of Revision Performed for Primary Total Conventional Hip Replacement

This analysis identifies the components used in the revision of the Avenir/Fitmore total conventional hip combination and compares it to the components used in the revision of all other total conventional hip prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total conventional hip prostheses i.e. is there a difference in the type of revision undertaken for the Avenir/Fitmore total conventional hip combination compared to all other total conventional hip prostheses.

Table 5: Primary Total Conventional Hip Replacement - Type of Revision (Follow-up Limited to 10.3 Years)

Type of Revision	Avenir/Fitmore		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Femoral Component	5	23.8	5687	32.6
Acetabular Component	4	19.0	3196	18.3
THR (Femoral/Acetabular)			1922	11.0
Cement Spacer			593	3.4
Removal of Prostheses			92	0.5
Reinsertion of Components			28	0.2
Bipolar Head and Femoral			7	0.0
Total Femoral			7	0.0
Saddle			1	0.0
N Major	9	42.9	11533	66.1
Head/Insert	12	57.1	4545	26.1
Head Only			900	5.2
Minor Components			280	1.6
Insert Only			183	1.0
Bipolar Only			2	0.0
Cement Only			1	0.0
Head/Neck			1	0.0
N Minor	12	57.1	5912	33.9
TOTAL	21	100.0	17445	100.0

Note: This table is restricted to revisions within 10.3 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 6**Revision Rates of Avenir/Fitmore Primary Total Conventional Hip Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of Avenir/Fitmore Primary Total Conventional Hip Replacement by Fixation

Fixation	N Revised	N Total
Cementless	21	372
TOTAL	21	372

TABLE 7**Revision Rates of Avenir/Fitmore Primary Total Conventional Hip Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this combination are listed.

Table 7: Revised Number of Avenir/Fitmore Primary Total Conventional Hip Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Metal/XLPE	21	372
TOTAL	21	372

TABLE 8**Revision Rates of Avenir/Fitmore Primary Total Conventional Hip Replacement by Approach**

This analysis is provided as some prostheses are used with a variety of surgical approaches. All surgical approaches used with this combination are listed.

Table 8: Revised Number of Avenir/Fitmore Primary Total Conventional Hip Replacement by Approach

Approach	N Revised	N Total
Anterior	0	27
Lateral	5	114
Posterior	13	217
TOTAL	18	358

Note: Excludes 14 procedures with no approach recorded

TABLE 9

Revision Rates of Primary Total Conventional Hip Replacement by State

This enables a state by state variation to be identified for the Avenir/Fitmore total conventional hip combination and provides the comparative data for each of the states for all other total conventional hip prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 9: Revised Number of Primary Total Conventional Hip Replacement by State

Component	State	N Revised	N Total
Avenir/Fitmore	NSW	21	372
Other Total Conventional Hip	NSW	5186	157335
	VIC	4859	140681
	QLD	3791	94582
	WA	2546	63265
	SA	1825	49398
	TAS	452	18198
	ACT/NT	569	14710
TOTAL		19249	538541

Note: Prostheses no longer used in 2023 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 10**Number of Revisions of Avenir/Fitmore Primary Total Conventional Hip Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the Avenir/Fitmore total conventional hip combination. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2023 has a maximum of one year to be revised, whereas a primary procedure performed in 2021 has a maximum of three years to be revised.

Table 10: Number of Revisions of Avenir/Fitmore Primary Total Conventional Hip Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2013	0	2
2014	3	7
2015	1	5
2016	0	46
2017	1	44
2018	4	42
2019	3	56
2020	3	41
2021	2	55
2022	1	41
2023	3	33
TOTAL	21	372

TABLE 11

Revision Rates of Avenir/Fitmore Primary Total Conventional Hip Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular Avenir/Fitmore prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Material	Coating
Femoral Stem					
Avenir	0106010001-0106010009	TITANIUM GRIT BLAST HA MULLER STANDARD STEM	NO	METAL	HA COATED
Avenir	0106010101-0106010109	TITANIUM GRIT BLAST HA MULLER LATERAL STEM	NO	METAL	HA COATED
Acetabular					
Fitmore	0100024542-0100024568	TITANIUM SHELL W/SCREW CONES	NO	METAL	

Table 11: Revised Number of Avenir/Fitmore Primary Total Conventional Hip Replacement by Catalogue Number Range

Femoral Stem Range	Acetabular Range	N Revised	N Total
0106010001-0106010009	0100024542-0100024568	17	304
0106010101-0106010109	0100024542-0100024568	4	68
TOTAL		21	372