

Journey Oxinium/Journey Total Knee Investigation

Note: This analysis compares the Journey Oxinium/Journey femoral/tibial combination with all other total knee prostheses.

This combination has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2022>.

Note: Procedures using prostheses with no recorded use in 2021 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Knee Replacement

The revision rate of the Journey Oxinium/Journey total knee combination is compared to all other total knee prostheses.

Table 1: Revision Rates of Primary Total Knee Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
Journey Oxinium/Journey	362	3033	30214	1.20 (1.08, 1.33)
Other Total Knee	26061	727695	4729125	0.55 (0.54, 0.56)
TOTAL	26423	730728	4759338	0.56 (0.55, 0.56)

Note: Prostheses no longer used in 2021 are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Journey Oxinium/Journey total knee combination is compared to all other total knee prostheses.

Table 2: Yearly Cumulative Percent Revision of Primary Total Knee Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs
Journey Oxinium/Journey	1.4 (1.0, 1.9)	3.4 (2.8, 4.1)	4.6 (3.9, 5.4)	5.6 (4.8, 6.5)	6.5 (5.6, 7.4)	7.4 (6.5, 8.4)	8.2 (7.3, 9.3)
Other Total Knee	1.0 (1.0, 1.0)	1.9 (1.9, 1.9)	2.5 (2.4, 2.5)	2.9 (2.9, 2.9)	3.2 (3.2, 3.3)	3.6 (3.5, 3.6)	3.9 (3.8, 3.9)

CPR	8 Yrs	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs
Journey Oxinium/Journey	9.1 (8.1, 10.2)	10.1 (9.1, 11.3)	11.0 (9.9, 12.2)	11.9 (10.8, 13.2)	13.1 (11.8, 14.5)	14.8 (13.3, 16.5)	15.0 (13.5, 16.7)
Other Total Knee	4.2 (4.1, 4.2)	4.5 (4.4, 4.5)	4.8 (4.7, 4.8)	5.1 (5.0, 5.2)	5.4 (5.3, 5.5)	5.7 (5.7, 5.8)	6.1 (6.0, 6.1)

CPR	15 Yrs	16 Yrs	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs
Journey Oxinium/Journey	17.1 (14.5, 20.2)						
Other Total Knee	6.4 (6.3, 6.6)	6.9 (6.7, 7.0)	7.3 (7.1, 7.4)	7.6 (7.4, 7.8)	7.9 (7.7, 8.1)	8.2 (7.9, 8.4)	8.2 (8.0, 8.5)

Note: Prostheses no longer used in 2021 are excluded from the comparator.


FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Journey Oxinium/Journey total knee combination is compared to all other total knee prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Knee Replacement

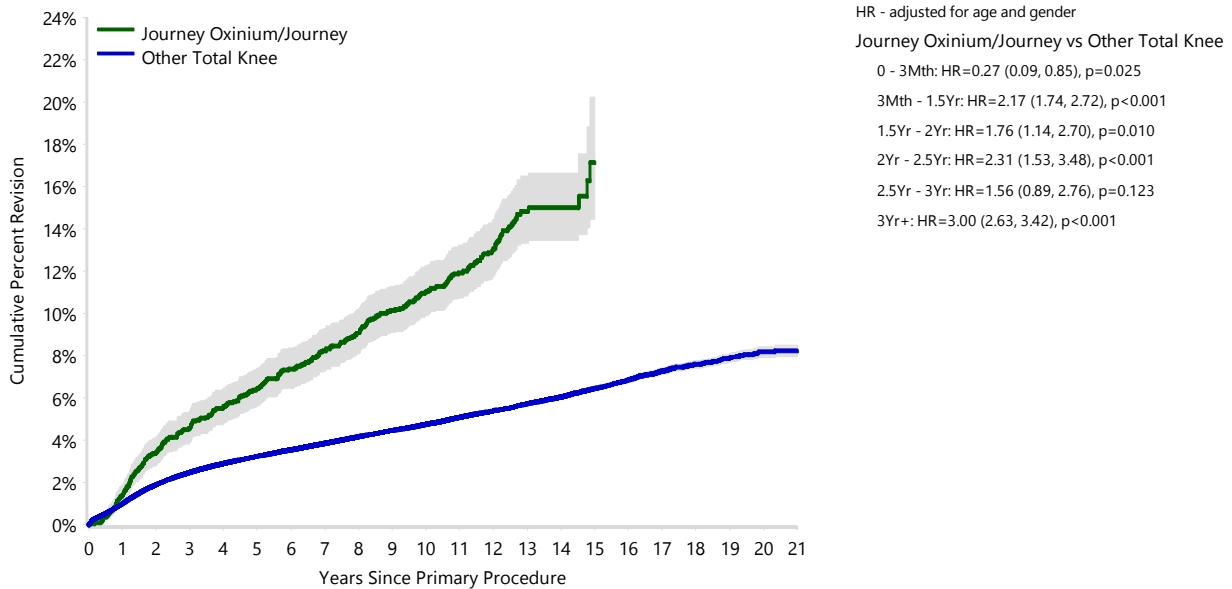

Number at Risk	0 Yr	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs	9 Yrs	10 Yrs
Journey Oxinium/Journey	3033	2972	2883	2813	2755	2692	2620	2510	2429	2076	1702
Other Total Knee	727695	657528	592760	527219	464041	403691	347132	293768	245752	202649	163502

Number at Risk	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs
Journey Oxinium/Journey	1361	994	583	273	72	0	0	0	0	0	0
Other Total Knee	128843	99109	75527	56481	41660	29601	19593	11953	6490	2687	605

Note: Prostheses no longer used in 2021 are excluded from the comparator.

TABLE 3**Primary Diagnosis for Revised Primary Total Knee Replacement**

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total knee prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Knee Replacement

Primary Diagnosis	Journey Oxinium/Journey		Other Total Knee	
	Number	Percent	Number	Percent
Osteoarthritis	360	99.4	25251	96.9
Rheumatoid Arthritis	1	0.3	331	1.3
Other Inflammatory Arthritis	1	0.3	161	0.6
Tumour			151	0.6
Osteonecrosis			98	0.4
Fracture			49	0.2
Other			19	0.1
Chondrocalcinosis			1	0.0
TOTAL	362	100.0	26061	100.0

Note: Prostheses no longer used in 2021 are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Knee Replacement - Reason for Revision (Follow-up Limited to 15.5 Years)

Revision Diagnosis	Journey Oxinium/Journey			Other Total Knee		
	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	45	1.5	12.4	6941	1.0	26.9
Loosening	86	2.8	23.8	5758	0.8	22.3
Instability	39	1.3	10.8	2462	0.3	9.6
Pain	34	1.1	9.4	2050	0.3	8.0
Patellofemoral Pain	48	1.6	13.3	2039	0.3	7.9
Patella Erosion	37	1.2	10.2	1666	0.2	6.5
Arthrofibrosis	4	0.1	1.1	995	0.1	3.9
Fracture	8	0.3	2.2	923	0.1	3.6
Malalignment	3	0.1	0.8	600	0.1	2.3
Wear Tibial Insert	4	0.1	1.1	340	0.0	1.3
Lysis	4	0.1	1.1	328	0.0	1.3
Incorrect Sizing	2	0.1	0.6	258	0.0	1.0
Patella Maltracking	1	0.0	0.3	181	0.0	0.7
Bearing Dislocation	3	0.1	0.8	152	0.0	0.6
Implant Breakage Tibial Insert	35	1.2	9.7	145	0.0	0.6
Implant Breakage Patella				133	0.0	0.5
Metal Related Pathology	1	0.0	0.3	114	0.0	0.4
Prosthesis Dislocation	1	0.0	0.3	79	0.0	0.3
Synovitis	4	0.1	1.1	78	0.0	0.3
Osteonecrosis				58	0.0	0.2
Implant Breakage Tibial				40	0.0	0.2
Implant Breakage Femoral				38	0.0	0.1
Wear Patella	1	0.0	0.3	31	0.0	0.1
Tumour				27	0.0	0.1
Heterotopic Bone				15	0.0	0.1
Wear Tibial				11	0.0	0.0
Progression Of Disease				6	0.0	0.0
Patella Dislocation				2	0.0	0.0
Wear Femoral				2	0.0	0.0
Incorrect Side				1	0.0	0.0
Other	2	0.1	0.6	301	0.0	1.2
N Revision	362	11.9	100.0	25774	3.5	100.0
N Primary	3033			727695		

Note: This table is restricted to revisions within 15.5 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2021 are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Knee Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the Journey Oxinium/Journey total knee combination. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total knee prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Knee Replacement

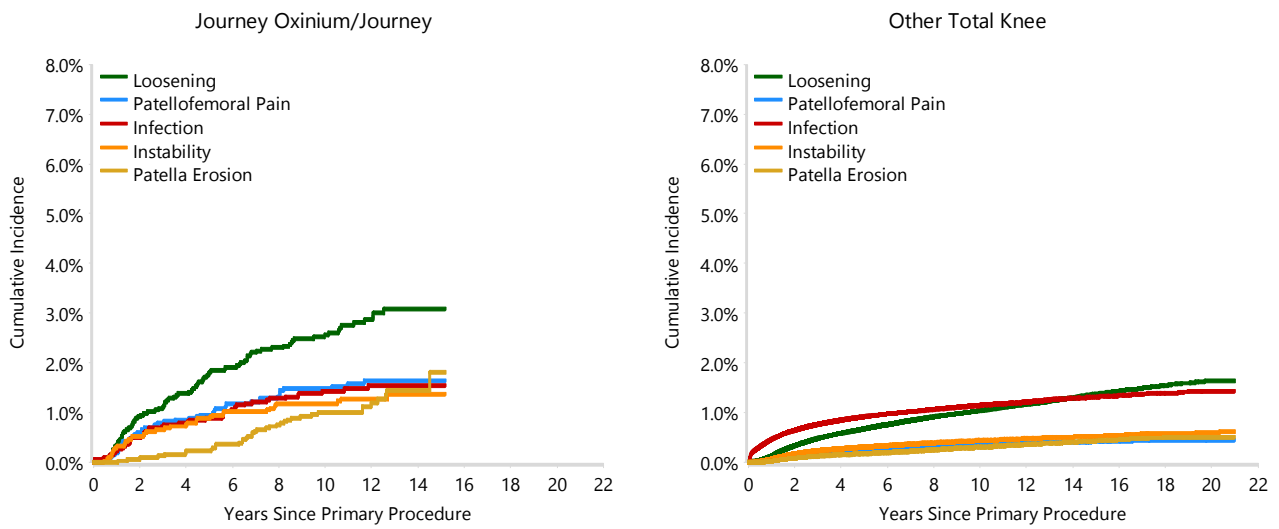


TABLE 5

Type of Revision Performed for Primary Total Knee Replacement

This analysis identifies the components used in the revision of the Journey Oxinium/Journey total knee combination and compares it to the components used in the revision of all other total knee prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total knee prostheses i.e. is there a difference in the type of revision undertaken for the Journey Oxinium/Journey total knee combination compared to all other total knee prostheses.

Table 5: Primary Total Knee Replacement - Type of Revision (Follow-up Limited to 15.5 Years)

Type of Revision	Journey Oxinium/Journey		Other Total Knee	
	Number	Percent	Number	Percent
TKR (Tibial/Femoral)	62	17.1	6296	24.4
Tibial Component	31	8.6	2094	8.1
Cement Spacer	9	2.5	1352	5.2
Femoral Component	5	1.4	1310	5.1
Removal of Prostheses			149	0.6
Total Femoral			20	0.1
Reinsertion of Components			11	0.0
N Major	107	29.6	11232	43.6
Insert Only	97	26.8	7069	27.4
Patella Only	109	30.1	4759	18.5
Insert/Patella	49	13.5	2641	10.2
Minor Components			59	0.2
Cement Only			14	0.1
N Minor	255	70.4	14542	56.4
TOTAL	362	100.0	25774	100.0

Note: This table is restricted to revisions within 15.5 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2021 are excluded from the comparator.

TABLE 6**Revision Rates of Journey Oxinium/Journey Primary Total Knee Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of Journey Oxinium/Journey Primary Total Knee Replacement by Fixation

Fixation	N Revised	N Total
Cemented	362	3032
Cementless	0	1
TOTAL	362	3033

TABLE 7**Revision Rates of Journey Oxinium/Journey Primary Total Knee Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this combination are listed.

Table 7: Revised Number of Journey Oxinium/Journey Primary Total Knee Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Non XLPE	362	3032
Unknown	0	1
TOTAL	362	3033

TABLE 8**Revision Rates of Journey Oxinium/Journey Primary Total Knee Replacement by Bearing Mobility**

This analysis is provided as some prostheses are combined with a variety of bearing mobilities. All bearing mobilities used with this combination are listed.

Table 8: Revised Number of Journey Oxinium/Journey Primary Total Knee Replacement by Bearing Mobility

Bearing Mobility	N Revised	N Total
Fixed	362	3032
Unknown	0	1
TOTAL	362	3033

TABLE 9**Revision Rates of Journey Oxinium/Journey Primary Total Knee Replacement by Stability**

This analysis is provided as some prostheses are combined with a variety of stabilities. All stabilities used with this combination are listed.

Table 9: Revised Number of Journey Oxinium/Journey Primary Total Knee Replacement by Stability

Stability	N Revised	N Total
Posterior Stabilised	362	3032
Unknown	0	1
TOTAL	362	3033

TABLE 10

Revision Rates of Primary Total Knee Replacement by State

This enables a state by state variation to be identified for the Journey Oxinium/Journey total knee combination and provides the comparative data for each of the states for all other total knee prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 10: Revised Number of Primary Total Knee Replacement by State

Component	State	N Revised	N Total
Journey Oxinium/Journey	NSW	23	235
	VIC	80	688
	QLD	145	1557
	WA	27	108
	SA	72	396
	ACT/NT	15	49
Other Total Knee	NSW	7722	253121
	VIC	5553	144487
	QLD	5690	153171
	WA	3235	77905
	SA	2837	63440
	TAS	418	16885
	ACT/NT	606	18686
TOTAL		26423	730728

Note: Prostheses no longer used in 2021 are excluded from the comparator.

TABLE 11**Number of Revisions of Journey Oxinium/Journey Primary Total Knee Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the Journey Oxinium/Journey total knee combination. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2021 has a maximum of one year to be revised, whereas a primary procedure performed in 2019 has a maximum of three years to be revised.

Table 11: Number of Revisions of Journey Oxinium/Journey Primary Total Knee Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2006	21	134
2007	56	337
2008	88	541
2009	64	555
2010	52	464
2011	40	334
2012	17	343
2013	24	325
TOTAL	362	3033

TABLE 12

Revision Rates of Journey Oxinium/Journey Primary Total Knee Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular Journey Oxinium/Journey prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Fixation
Femoral				
Journey Oxinium	74021110-74021129	NONPOROUS OXINIUM BI-CRUCIATE STABILIZED FEMORAL COMPONENT	YES	
Tibial				
Journey	74022211-74022228	NONPOROUS TIBIAL BASEPLATE	YES	POLISHED

Table 12: Revised Number of Journey Oxinium/Journey Primary Total Knee Replacement by Catalogue Number Range

Femoral Range	Tibial Range	N Revised	N Total
74021110-74021129	74022211-74022228	362	3033
TOTAL		362	3033