

HACTIV Total Conventional Hip Investigation

Note: This analysis compares the HACTIV femoral stem prosthesis with all other total conventional hip prostheses.

This prosthesis has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2025>.

Note: Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator. Procedures using prostheses with no recorded use in 2024 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Conventional Hip Replacement

The revision rate of the HACTIV total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 1: Revision Rates of Primary Total Conventional Hip Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
HACTIV	126	3052	14993	0.84 (0.70, 1.00)
Other Total Conventional Hip	19368	549150	3537812	0.55 (0.54, 0.56)
TOTAL	19494	552202	3552805	0.55 (0.54, 0.56)

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 2**Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement**

The yearly cumulative percent revision of the HACTIV total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 2: Yearly Cumulative Percent Revision (95% CI) of Primary Total Conventional Hip Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs
HACTIV	2.6 (2.1, 3.2)	3.3 (2.7, 4.0)	3.6 (2.9, 4.3)	3.7 (3.1, 4.5)	4.0 (3.3, 4.8)	4.4 (3.7, 5.3)	4.7 (3.9, 5.7)	5.1 (4.2, 6.1)
Other Total Conventional Hip	1.7 (1.7, 1.8)	2.2 (2.1, 2.2)	2.5 (2.4, 2.5)	2.8 (2.7, 2.8)	3.0 (3.0, 3.1)	3.3 (3.3, 3.4)	3.6 (3.5, 3.6)	3.8 (3.8, 3.9)
CPR	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs
HACTIV	5.6 (4.5, 7.0)	6.0 (4.7, 7.7)	6.9 (5.0, 9.5)	6.9 (5.0, 9.5)				
Other Total Conventional Hip	4.2 (4.1, 4.2)	4.4 (4.4, 4.5)	4.8 (4.7, 4.8)	5.2 (5.1, 5.3)	5.5 (5.4, 5.6)	5.9 (5.8, 6.0)	6.3 (6.2, 6.4)	6.7 (6.6, 6.9)
CPR	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs	
HACTIV								
Other Total Conventional Hip	7.1 (6.9, 7.2)	7.4 (7.3, 7.6)	7.9 (7.7, 8.1)	8.3 (8.0, 8.5)	8.8 (8.5, 9.1)	9.3 (9.0, 9.7)	9.9 (9.4, 10.4)	


Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 1**Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement**

The yearly cumulative percent revision of the HACTIV total conventional hip prosthesis is compared to all other total conventional hip prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Conventional Hip Replacement

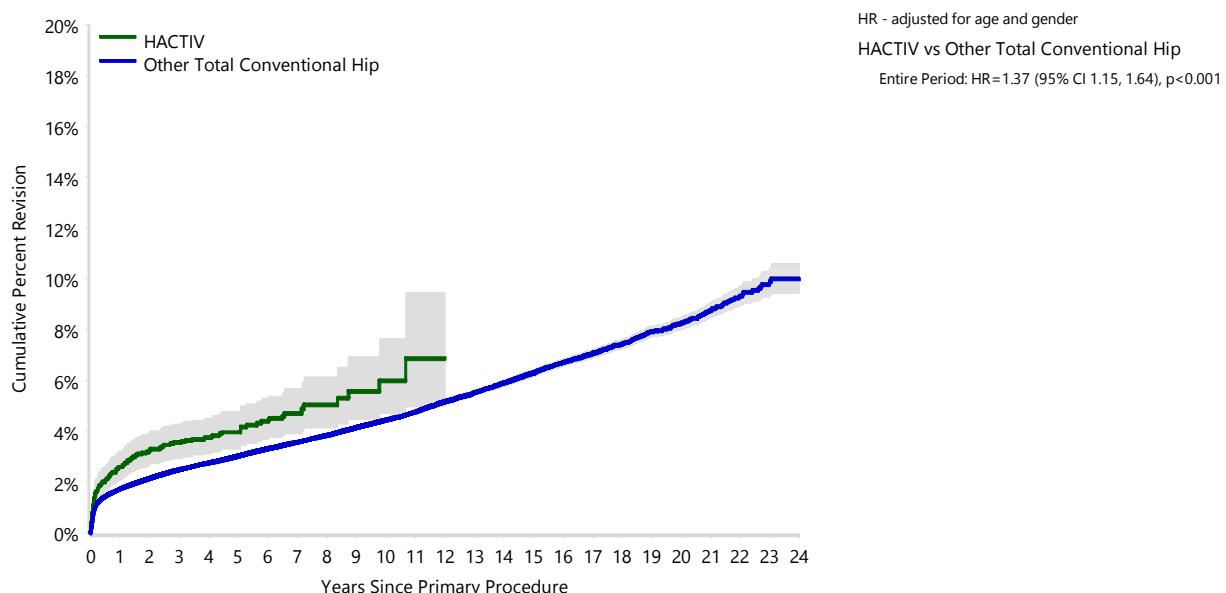

Number at Risk	0 Yr	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs
HACTIV	3052	2732	2471	2251	1839	1423	1063	639	417	322	192	101
Other Total Conventional Hip	549150	485030	430385	381988	335403	294415	253909	216510	181839	150077	121981	99296
Number at Risk	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
HACTIV	54	13	2	0	0	0	0	0	0	0	0	0
Other Total Conventional Hip	80188	63995	49888	37936	28064	20581	15102	10871	7426	4536	2346	851

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 3**Primary Diagnosis for Revised Primary Total Conventional Hip Replacement**

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total conventional hip prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Conventional Hip Replacement

Primary Diagnosis	HACTIV		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Osteoarthritis	119	94.4	16057	82.9
Fractured Neck Of Femur	1	0.8	1435	7.4
Osteonecrosis	2	1.6	854	4.4
Developmental Dysplasia	2	1.6	311	1.6
Rheumatoid Arthritis			210	1.1
Failed Internal Fixation			157	0.8
Tumour			148	0.8
Other Inflammatory Arthritis	1	0.8	111	0.6
Fracture/Dislocation			53	0.3
Other			19	0.1
Arthrodesis Takedown	1	0.8	13	0.1
TOTAL	126	100.0	19368	100.0

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 4**Reasons for Revision**

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Conventional Hip Replacement - Reason for Revision (Follow-up Limited to 14.1 Years)

Revision Diagnosis	Number	HACTIV		Other Total Conventional Hip		
		% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	31	1.0	24.6	4668	0.9	24.9
Prosthesis Dislocation/Instability	33	1.1	26.2	4293	0.8	22.9
Fracture	27	0.9	21.4	4153	0.8	22.2
Loosening	15	0.5	11.9	3504	0.6	18.7
Pain	5	0.2	4.0	314	0.1	1.7
Leg Length Discrepancy	1	0.0	0.8	296	0.1	1.6
Malposition	2	0.1	1.6	264	0.0	1.4
Implant Breakage Stem	1	0.0	0.8	186	0.0	1.0
Lysis	1	0.0	0.8	172	0.0	0.9
Implant Breakage Acetabular Insert	1	0.0	0.8	121	0.0	0.6
Incorrect Sizing	1	0.0	0.8	97	0.0	0.5
Wear Acetabular Insert				80	0.0	0.4
Metal Related Pathology	2	0.1	1.6	73	0.0	0.4
Implant Breakage Acetabular				66	0.0	0.4
Wear Head				41	0.0	0.2
Tumour				40	0.0	0.2
Heterotopic Bone				27	0.0	0.1
Implant Breakage Head				27	0.0	0.1
Wear Acetabulum				9	0.0	0.0
Osteonecrosis				3	0.0	0.0
Synovitis				1	0.0	0.0
Other	6	0.2	4.8	303	0.1	1.6
N Revision	126	4.1	100.0	18738	3.4	100.0
N Primary	3052			549150		

Note: This table is restricted to revisions within 14.1 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 2**Cumulative Incidence Revision Diagnosis of Primary Total Conventional Hip Replacement**

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the HACTIV total conventional hip prosthesis. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total conventional hip prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Conventional Hip Replacement

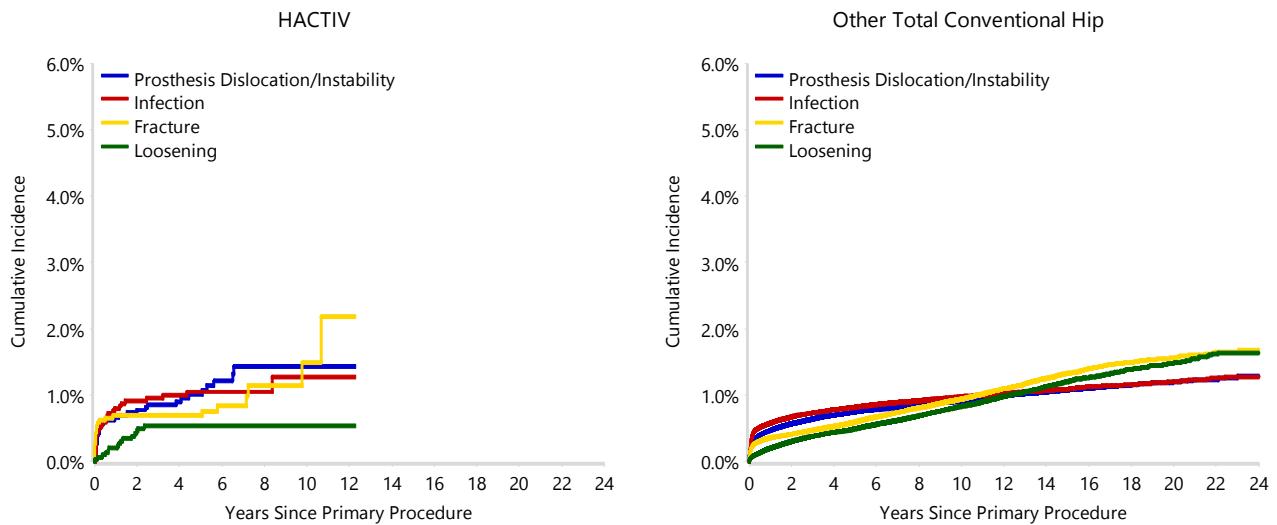


TABLE 5**Type of Revision Performed for Primary Total Conventional Hip Replacement**

This analysis identifies the components used in the revision of the HACTIV total conventional hip prosthesis and compares it to the components used in the revision of all other total conventional hip prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total conventional hip prostheses i.e. is there a difference in the type of revision undertaken for the HACTIV total conventional hip prosthesis compared to all other total conventional hip prostheses.

Table 5: Primary Total Conventional Hip Replacement - Type of Revision (Follow-up Limited to 14.1 Years)

Type of Revision	HACTIV		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Femoral Component	32	25.4	6325	33.8
Acetabular Component	44	34.9	3207	17.1
THR (Femoral/Aacetabular)	16	12.7	2117	11.3
Cement Spacer	4	3.2	583	3.1
Removal of Prostheses			95	0.5
Reinsertion of Components			29	0.2
Total Femoral			12	0.1
Bipolar Head and Femoral			9	0.0
N Major	96	76.2	12377	66.1
Head/Insert	27	21.4	4979	26.6
Head Only	3	2.4	909	4.9
Minor Components			294	1.6
Insert Only			176	0.9
Bipolar Only			1	0.0
Cement Only			1	0.0
Head/Neck			1	0.0
N Minor	30	23.8	6361	33.9
TOTAL	126	100.0	18738	100.0

Note: This table is restricted to revisions within 14.1 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 6**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Fixation

Fixation	N Revised	N Total
Cementless	125	3048
Hybrid (Femur Cemented)	1	3
Reverse Hybrid (Femur Cementless)	0	1
TOTAL	126	3052

TABLE 7**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this prosthesis are listed.

Table 7: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Ceramic/Ceramic	17	357
Ceramic/Non XLPE	17	986
Ceramic/XLPE	75	1312
Ceramic/XLPE + Antioxidant	5	175
Metal/Non XLPE	7	116
Metal/XLPE	5	101
Metal/XLPE + Antioxidant	0	5
TOTAL	126	3052

TABLE 8**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Approach**

This analysis is provided as some prostheses are used with a variety of surgical approaches. All surgical approaches used with this prosthesis are listed.

Table 8: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Approach

Approach	N Revised	N Total
Anterior	17	427
Lateral	15	373
Posterior	75	1964
TOTAL	107	2764

Note: Excludes 288 procedures with no approach recorded

TABLE 9**Number of Revisions of HACTIV Primary Total Conventional Hip Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the HACTIV total conventional hip prosthesis. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2024 has a maximum of one year to be revised, whereas a primary procedure performed in 2022 has a maximum of three years to be revised.

Table 9: Number of Revisions of HACTIV Primary Total Conventional Hip Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2010	0	2
2011	4	19
2012	1	63
2013	4	61
2014	9	117
2015	3	146
2016	1	96
2017	17	240
2018	23	452
2019	24	388
2020	17	418
2021	13	406
2022	3	194
2023	5	225
2024	2	225
TOTAL	126	3052

TABLE 10**Revision Rates of HACTIV Primary Total Conventional Hip Replacement by Component**

A prosthesis may be combined with multiple components. This analysis has been undertaken to determine if the revision rate varies according to the component with which it is combined.

Table 10: Revised Number of HACTIV Primary Total Conventional Hip Replacement by Acetabular Component

Acetabular Component	N Revised	N Total
Austral	3	62
Cer-Met	1	12
Delta-TT	9	130
FMP	0	13
Fin II	1	41
Furlong	1	18
G7	0	1
Logical G	79	1384
Marathon	0	1
PINNACLE	1	9
R3	0	5
Saturne	25	1151
Trabecular Metal (Shell)	0	2
Trident (Shell)	1	1
Trident/Titanium (Shell)	0	14
Trinity	5	208
TOTAL	126	3052