

Scorpio NRG PS (cementless)/Series 7000 (cementless) Total Knee Investigation

Note: This analysis compares the Scorpio NRG PS (cless)/Series 7000 (cless) femoral/tibial combination with all other total knee prostheses.

This combination has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2025>.

Note: Procedures using prostheses with no recorded use in 2024 are excluded from the comparator.

TABLE 1

Revision Rate of Primary Total Knee Replacement

The revision rate of the Scorpio NRG PS (cless)/Series 7000 (cless) total knee combination is compared to all other total knee prostheses.

Table 1: Revision Rates of Primary Total Knee Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
Scorpio NRG PS (cless)/Series 7000 (cless)	96	1172	13166	0.73 (0.59, 0.89)
Other Total Knee	24707	721061	4535539	0.54 (0.54, 0.55)
TOTAL	24803	722233	4548705	0.55 (0.54, 0.55)

Note: Prostheses no longer used in 2024 are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Scorpio NRG PS (cless)/Series 7000 (cless) total knee combination is compared to all other total knee prostheses.

Table 2: Yearly Cumulative Percent Revision (95% CI) of Primary Total Knee Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs
Scorpio NRG PS (cless)/Series 7000 (cless)	1.2 (0.7, 2.0)	3.4 (2.5, 4.6)	4.9 (3.8, 6.3)	5.6 (4.5, 7.1)	6.2 (4.9, 7.7)	6.5 (5.2, 8.1)	6.6 (5.3, 8.2)	6.8 (5.5, 8.4)
Other Total Knee	1.0 (1.0, 1.0)	1.8 (1.8, 1.9)	2.4 (2.4, 2.4)	2.8 (2.8, 2.8)	3.2 (3.1, 3.2)	3.5 (3.4, 3.5)	3.8 (3.7, 3.8)	4.1 (4.0, 4.2)

CPR	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs
Scorpio NRG PS (cless)/Series 7000 (cless)	7.0 (5.7, 8.7)	7.4 (6.0, 9.1)	7.9 (6.5, 9.7)	8.1 (6.6, 9.9)	8.1 (6.6, 9.9)	8.7 (7.1, 10.6)	9.5 (7.7, 11.7)	9.5 (7.7, 11.7)
Other Total Knee	4.4 (4.3, 4.5)	4.7 (4.7, 4.8)	5.1 (5.0, 5.1)	5.4 (5.3, 5.5)	5.7 (5.6, 5.8)	6.0 (5.9, 6.1)	6.4 (6.3, 6.5)	6.8 (6.7, 7.0)

CPR	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
Scorpio NRG PS (cless)/Series 7000 (cless)	12.2 (8.3, 17.8)						
Other Total Knee	7.3 (7.1, 7.4)	7.6 (7.4, 7.8)	7.9 (7.7, 8.1)	8.1 (7.9, 8.3)	8.4 (8.1, 8.6)	8.5 (8.2, 8.8)	8.6 (8.3, 8.9)

Note: Prostheses no longer used in 2024 are excluded from the comparator.


FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Knee Replacement

The yearly cumulative percent revision of the Scorpio NRG PS (cless)/Series 7000 (cless) total knee combination is compared to all other total knee prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Knee Replacement

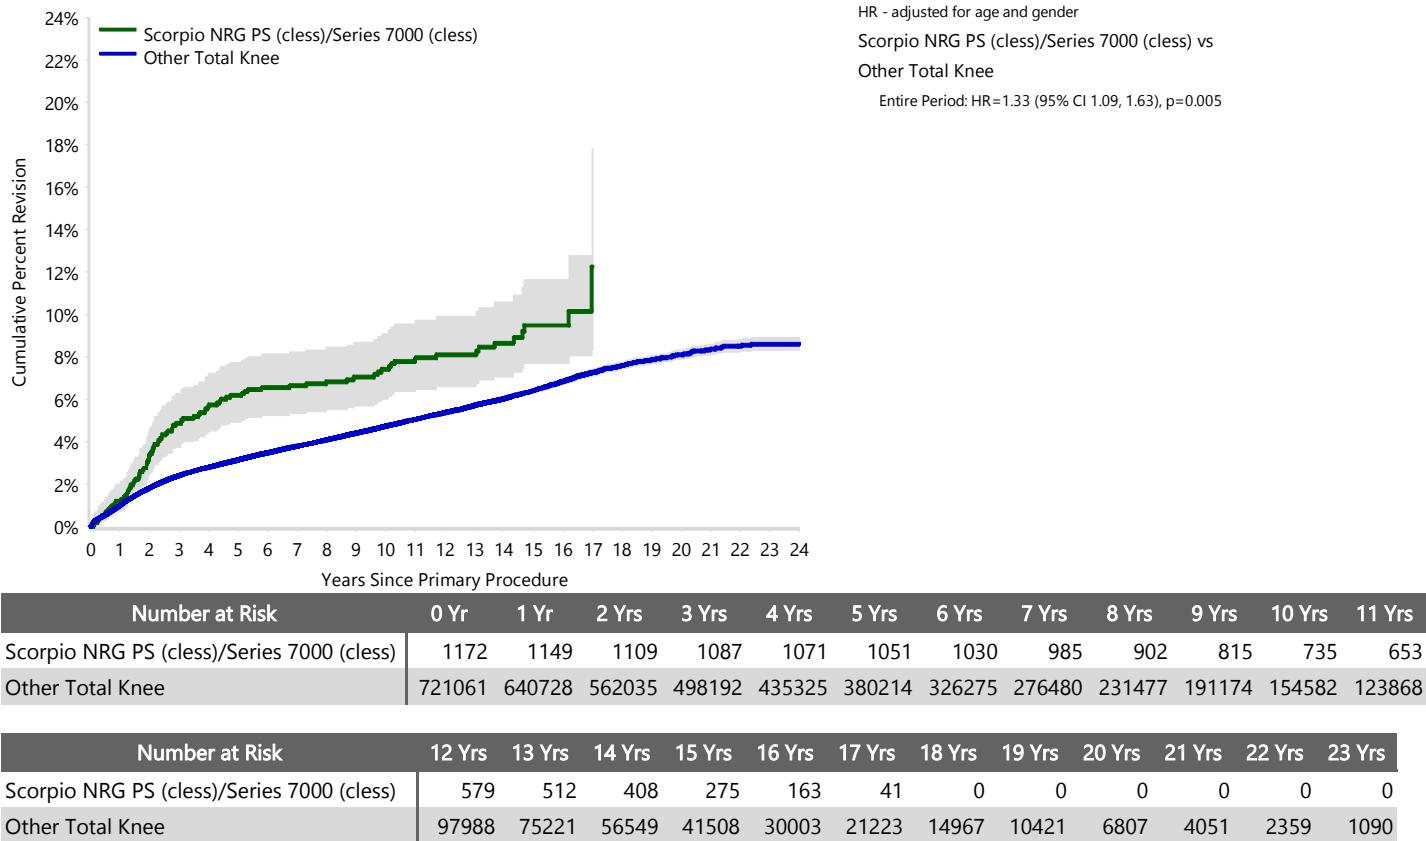

Note: Prostheses no longer used in 2024 are excluded from the comparator.

TABLE 3**Primary Diagnosis for Revised Primary Total Knee Replacement**

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total knee prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Knee Replacement

Primary Diagnosis	Scorpio NRG PS (class)/Series 7000 (class)		Other Total Knee	
	Number	Percent	Number	Percent
Osteoarthritis	96	100.0	23890	96.7
Rheumatoid Arthritis			301	1.2
Tumour			192	0.8
Other Inflammatory Arthritis			158	0.6
Osteonecrosis			90	0.4
Fracture			50	0.2
Other			25	0.1
Chondrocalcinosis			1	0.0
TOTAL	96	100.0	24707	100.0

Note: Prostheses no longer used in 2024 are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Knee Replacement - Reason for Revision (Follow-up Limited to 17.8 Years)

Revision Diagnosis	Scorpio NRG PS (class)/Series 7000 (class)			Other Total Knee		
	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	19	1.6	19.8	7081	1.0	28.8
Loosening	42	3.6	43.8	5231	0.7	21.3
Instability	4	0.3	4.2	2533	0.4	10.3
Patella Erosion	4	0.3	4.2	1805	0.3	7.3
Pain	8	0.7	8.3	1756	0.2	7.1
Patellofemoral Pain	1	0.1	1.0	1478	0.2	6.0
Arthrofibrosis	5	0.4	5.2	1047	0.1	4.3
Fracture	2	0.2	2.1	1006	0.1	4.1
Malalignment	1	0.1	1.0	488	0.1	2.0
Wear Tibial Insert	2	0.2	2.1	318	0.0	1.3
Lysis				261	0.0	1.1
Incorrect Sizing	1	0.1	1.0	210	0.0	0.9
Implant Breakage Tibial Insert	5	0.4	5.2	203	0.0	0.8
Patella Maltracking				175	0.0	0.7
Bearing Dislocation				141	0.0	0.6
Implant Breakage Patella				131	0.0	0.5
Metal Related Pathology				101	0.0	0.4
Prosthesis Dislocation				70	0.0	0.3
Synovitis				59	0.0	0.2
Osteonecrosis				46	0.0	0.2
Implant Breakage Femoral				43	0.0	0.2
Wear Patella	1	0.1	1.0	43	0.0	0.2
Implant Breakage Tibial				34	0.0	0.1
Tumour				30	0.0	0.1
Heterotopic Bone				14	0.0	0.1
Progression Of Disease				8	0.0	0.0
Wear Tibial				6	0.0	0.0
Incorrect Side				1	0.0	0.0
Patella Dislocation				1	0.0	0.0
Wear Femoral				1	0.0	0.0
Other	1	0.1	1.0	295	0.0	1.2
N Revision	96	8.2	100.0	24616	3.4	100.0
N Primary	1172			721061		

Note: This table is restricted to revisions within 17.8 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2024 are excluded from the comparator.

FIGURE 2**Cumulative Incidence Revision Diagnosis of Primary Total Knee Replacement**

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the Scorpio NRG PS (cless)/Series 7000 (cless) total knee combination. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total knee prostheses.

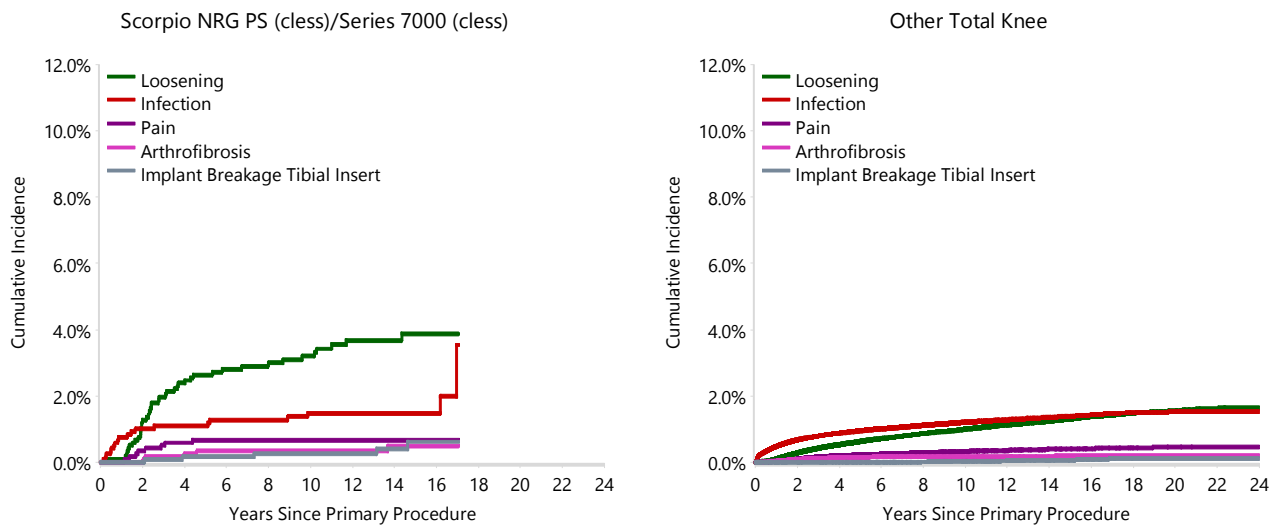
Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Knee Replacement

TABLE 5**Type of Revision Performed for Primary Total Knee Replacement**

This analysis identifies the components used in the revision of the Scorpio NRG PS (class)/Series 7000 (class) total knee combination and compares it to the components used in the revision of all other total knee prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total knee prostheses i.e. is there a difference in the type of revision undertaken for the Scorpio NRG PS (class)/Series 7000 (class) total knee combination compared to all other total knee prostheses.

Table 5: Primary Total Knee Replacement - Type of Revision (Follow-up Limited to 17.8 Years)

Type of Revision	Scorpio NRG PS (class)/Series 7000 (class)		Other Total Knee	
	Number	Percent	Number	Percent
TKR (Tibial/Femoral)	19	19.8	5871	23.9
Tibial Component	9	9.4	1802	7.3
Femoral Component	3	3.1	1184	4.8
Cement Spacer	8	8.3	1081	4.4
Removal of Prostheses			124	0.5
Total Femoral			22	0.1
Reinsertion of Components			7	0.0
N Major	39	40.6	10091	41.0
Insert Only	23	24.0	7655	31.1
Patella Only	11	11.5	4154	16.9
Insert/Patella	23	24.0	2644	10.7
Minor Components			63	0.3
Cement Only			9	0.0
N Minor	57	59.4	14525	59.0
TOTAL	96	100.0	24616	100.0

Note: This table is restricted to revisions within 17.8 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2024 are excluded from the comparator.

TABLE 6**Revision Rates of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Fixation

Fixation	N Revised	N Total
Cemented	0	2
Cementless	92	1141
Hybrid (Tibial Cemented)	4	28
Hybrid (Tibial Cementless)	0	1
TOTAL	96	1172

TABLE 7**Revision Rates of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this combination are listed.

Table 7: Revised Number of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Non XLPE	10	106
XLPE	86	1066
TOTAL	96	1172

TABLE 8**Revision Rates of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Bearing Mobility**

This analysis is provided as some prostheses are combined with a variety of bearing mobilities. All bearing mobilities used with this combination are listed.

Table 8: Revised Number of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Bearing Mobility

Bearing Mobility	N Revised	N Total
Fixed	96	1172
TOTAL	96	1172

TABLE 9**Revision Rates of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Stability**

This analysis is provided as some prostheses are combined with a variety of stabilities. All stabilities used with this combination are listed.

Table 9: Revised Number of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Stability

Stability	N Revised	N Total
Posterior Stabilised	96	1172
TOTAL	96	1172

TABLE 10

Revision Rates of Primary Total Knee Replacement by State

This enables a state by state variation to be identified for the Scorpio NRG PS (cless)/Series 7000 (cless) total knee combination and provides the comparative data for each of the states for all other total knee prostheses.

The purpose of this analysis is to determine if the higher than anticipated rate of revision has widespread distribution between states. If there is widespread distribution then the reason for the higher than anticipated rate of revision is unlikely to be surgeon specific. If the prosthesis has been used in only a small number of states it is not possible to distinguish if the higher than anticipated rate of revision is related to the prosthesis, surgeon, technique or patient.

Table 10: Revised Number of Primary Total Knee Replacement by State

Component	State	N Revised	N Total
Scorpio NRG PS (cless)/Series 7000 (cless)	NSW	16	195
	VIC	30	642
	QLD	0	4
	WA	46	279
	TAS	4	52
Other Total Knee	NSW	6834	236304
	VIC	5457	148735
	QLD	5317	152558
	WA	3259	85158
	SA	2886	66544
	TAS	390	13242
	ACT/NT	564	18520
TOTAL		24803	722233

Note: Prostheses no longer used in 2024 are excluded from the comparator.

TABLE 11**Number of Revisions of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the Scorpio NRG PS (cless)/Series 7000 (cless) total knee combination. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2024 has a maximum of one year to be revised, whereas a primary procedure performed in 2022 has a maximum of three years to be revised.

Table 11: Number of Revisions of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2007	7	76
2008	21	185
2009	28	171
2010	13	166
2011	10	114
2012	2	67
2013	2	71
2014	5	76
2015	1	72
2016	3	77
2017	3	69
2018	1	28
TOTAL	96	1172

TABLE 12

Revision Rates of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Catalogue Number Range

Many prostheses have a number of catalogue ranges. The catalogue range is specific to particular design features; more than one catalogue range usually indicates a minor difference in design in a particular Scorpio NRG PS (cless)/Series 7000 (cless) prosthesis.

This analysis has been undertaken to determine if the revision rate varies according to the catalogue number range.

Model	Catalogue Range	Catalogue Description	Cement	Material	Coating	Fixation
Femoral						
Scorpio NRG PS	816403L-816413R	PS HA FEMORAL COMPONENT	NO		HA COATED	
Tibial						
Series 7000	71250003-71250013	SCORPIO COCR MICROSTRUCTURE BEADED TIBIAL BASEPLATE	NO			BEADED
Series 7000	71450003-71450013	SERIES 7000 STANDARD TIBIAL TRAY MICROSTRUCTURED COCR UHMWPE/PA COATED	NO	METAL	HA COATED	
Series 7000	75150003-75150013	SERIES 7000 STANDARD TIBIAL TRAY HA COATED	NO		HA COATED	

Table 12: Revised Number of Scorpio NRG PS (cless)/Series 7000 (cless) Primary Total Knee Replacement by Catalogue Number Range

Femoral Range	Tibial Range	N Revised	N Total
816403L-816413R	71250003-71250013	1	4
	71450003-71450013	54	375
	75150003-75150013	41	793
TOTAL		96	1172