

Versafitcup DM Total Conventional Hip Investigation

Note: This analysis compares the Versafitcup DM acetabular prosthesis with all other total conventional hip prostheses.

This prosthesis has been identified as having a significantly higher rate of revision. For a detailed explanation of the process used by the Registry that results in identification of prostheses that have a higher than anticipated rate of revision please refer to the Prostheses with Higher than Anticipated Rates of Revision chapter of the most recent AOANJRR Annual Report, <https://aoanjrr.sahmri.com/annual-reports-2025>.

Note: Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator. Procedures using prostheses with no recorded use in 2024 are excluded from the comparator.

TABLE 1
Revision Rate of Primary Total Conventional Hip Replacement

The revision rate of the Versafitcup DM total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 1: Revision Rates of Primary Total Conventional Hip Replacement

Component	N Revised	N Total	Obs. Years	Revisions/100 Obs. Yrs (95% CI)
Versafitcup DM	83	2447	9701	0.86 (0.68, 1.06)
Other Total Conventional Hip	19413	549739	3543015	0.55 (0.54, 0.56)
TOTAL	19496	552186	3552716	0.55 (0.54, 0.56)

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 2

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the Versafitcup DM total conventional hip prosthesis is compared to all other total conventional hip prostheses.

Table 2: Yearly Cumulative Percent Revision (95% CI) of Primary Total Conventional Hip Replacement

CPR	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs
Versafitcup DM	2.4 (1.8, 3.1)	3.0 (2.4, 3.8)	3.4 (2.7, 4.2)	3.5 (2.8, 4.4)	3.9 (3.1, 4.9)	3.9 (3.1, 4.9)	4.1 (3.2, 5.1)	4.8 (3.7, 6.2)
Other Total Conventional Hip	1.7 (1.7, 1.8)	2.2 (2.1, 2.2)	2.5 (2.4, 2.5)	2.8 (2.7, 2.8)	3.0 (3.0, 3.1)	3.3 (3.3, 3.4)	3.6 (3.5, 3.6)	3.9 (3.8, 3.9)

CPR	9 Yrs	10 Yrs	11 Yrs	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs
Versafitcup DM	4.8 (3.7, 6.2)							
Other Total Conventional Hip	4.2 (4.1, 4.2)	4.4 (4.4, 4.5)	4.8 (4.7, 4.8)	5.2 (5.1, 5.3)	5.5 (5.4, 5.6)	5.9 (5.8, 6.0)	6.3 (6.2, 6.4)	6.7 (6.6, 6.9)

CPR	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
Versafitcup DM							
Other Total Conventional Hip	7.1 (6.9, 7.2)	7.4 (7.3, 7.6)	7.9 (7.7, 8.1)	8.3 (8.0, 8.5)	8.8 (8.5, 9.1)	9.3 (9.0, 9.7)	9.9 (9.4, 10.5)

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.


FIGURE 1

Yearly Cumulative Percent Revision of Primary Total Conventional Hip Replacement

The yearly cumulative percent revision of the Versafitcup DM total conventional hip prosthesis is compared to all other total conventional hip prostheses. In addition, hazard ratios are reported.

Hazard ratios are reported for specific time periods during which the hazard ratio is constant. This is done to enable more specific and valid comparisons of the risk of revision over time. The pattern of variation in risk has important implications with respect to the underlying reasons for any difference.

Figure 1: Cumulative Percent Revision of Primary Total Conventional Hip Replacement

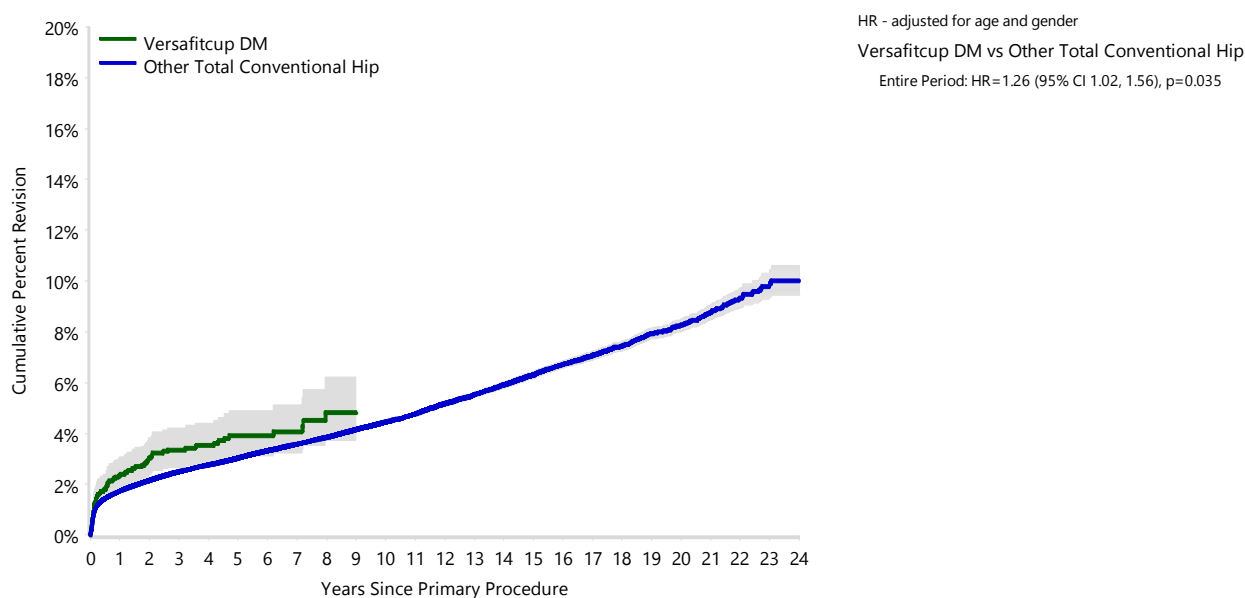

Number at Risk	0 Yr	1 Yr	2 Yrs	3 Yrs	4 Yrs	5 Yrs	6 Yrs	7 Yrs	8 Yrs	9 Yrs	10 Yrs	11 Yrs
Versafitcup DM	2447	2023	1623	1326	1070	830	663	477	307	149	32	16
Other Total Conventional Hip	549739	485722	431224	382911	336170	295006	254307	216669	181949	150249	122133	99369

Number at Risk	12 Yrs	13 Yrs	14 Yrs	15 Yrs	16 Yrs	17 Yrs	18 Yrs	19 Yrs	20 Yrs	21 Yrs	22 Yrs	23 Yrs
Versafitcup DM	11	3	0	0	0	0	0	0	0	0	0	0
Other Total Conventional Hip	80217	63996	49890	37936	28064	20581	15102	10871	7426	4536	2346	851

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 3**Primary Diagnosis for Revised Primary Total Conventional Hip Replacement**

This table identifies the diagnosis of the primary procedure which was subsequently revised. This information is provided as there is a variation on outcome depending on the primary diagnosis. It is therefore important when considering the reasons for a higher than anticipated rate of revision that there is identification of the primary diagnosis. This information should be compared to the primary diagnosis for the revisions of all other total conventional hip prostheses.

Table 3: Primary Diagnosis for Revised Primary Total Conventional Hip Replacement

Primary Diagnosis	Versafitcup DM		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Osteoarthritis	69	83.1	16108	83.0
Fractured Neck Of Femur	5	6.0	1431	7.4
Osteonecrosis	3	3.6	853	4.4
Developmental Dysplasia	3	3.6	311	1.6
Rheumatoid Arthritis	1	1.2	209	1.1
Failed Internal Fixation	2	2.4	155	0.8
Tumour			148	0.8
Other Inflammatory Arthritis			112	0.6
Fracture/Dislocation			53	0.3
Other			19	0.1
Arthrodesis Takedown			14	0.1
TOTAL	83	100.0	19413	100.0

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 4

Reasons for Revision

This is reported in two ways: a percentage of primary procedures revised and as a percentage of all revision procedures.

% Primaries Revised: This shows the proportional contribution of each revision diagnosis as a percentage of the total number of primary procedures. This percentage can be used to approximate the risk of being revised for that diagnosis. Differing percentages between groups, with the same distribution of follow up time, may identify problems of concern.

% Revisions: The number of revisions for each diagnosis is expressed as a percentage of the total number of revisions. This shows the distribution of reasons for revision within a group but cannot be used as a comparison between groups.

Table 4: Primary Total Conventional Hip Replacement - Reason for Revision (Follow-up Limited to 13.6 Years)

Revision Diagnosis	Versafitcup DM			Other Total Conventional Hip		
	Number	% Primaries Revised	% Revisions	Number	% Primaries Revised	% Revisions
Infection	24	1.0	28.9	4667	0.8	25.0
Prosthesis Dislocation/Instability	3	0.1	3.6	4309	0.8	23.1
Fracture	28	1.1	33.7	4119	0.7	22.1
Loosening	14	0.6	16.9	3469	0.6	18.6
Pain	2	0.1	2.4	317	0.1	1.7
Leg Length Discrepancy	1	0.0	1.2	296	0.1	1.6
Malposition	2	0.1	2.4	265	0.0	1.4
Implant Breakage Stem				184	0.0	1.0
Lysis				164	0.0	0.9
Implant Breakage Acetabular Insert				122	0.0	0.7
Incorrect Sizing	2	0.1	2.4	96	0.0	0.5
Metal Related Pathology				75	0.0	0.4
Wear Acetabular Insert				75	0.0	0.4
Implant Breakage Acetabular	1	0.0	1.2	65	0.0	0.3
Wear Head				40	0.0	0.2
Tumour				39	0.0	0.2
Heterotopic Bone				27	0.0	0.1
Implant Breakage Head				27	0.0	0.1
Wear Acetabulum				8	0.0	0.0
Osteonecrosis				3	0.0	0.0
Synovitis				1	0.0	0.0
Other	6	0.2	7.2	303	0.1	1.6
N Revision	83	3.4	100.0	18671	3.4	100.0
N Primary	2447			549739		

Note: This table is restricted to revisions within 13.6 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

FIGURE 2

Cumulative Incidence Revision Diagnosis of Primary Total Conventional Hip Replacement

This figure details the cumulative incidence of the most common reasons for revision. The five most common reasons for revision are included as long as each of these reasons account for more than 10 procedures or at least 5% of all revisions for the Versafitcup DM total conventional hip prosthesis. A comparative graph is provided of the cumulative incidence for the same reasons for revisions for all other total conventional hip prostheses.

Figure 2: Cumulative Incidence Revision Diagnosis for Primary Total Conventional Hip Replacement

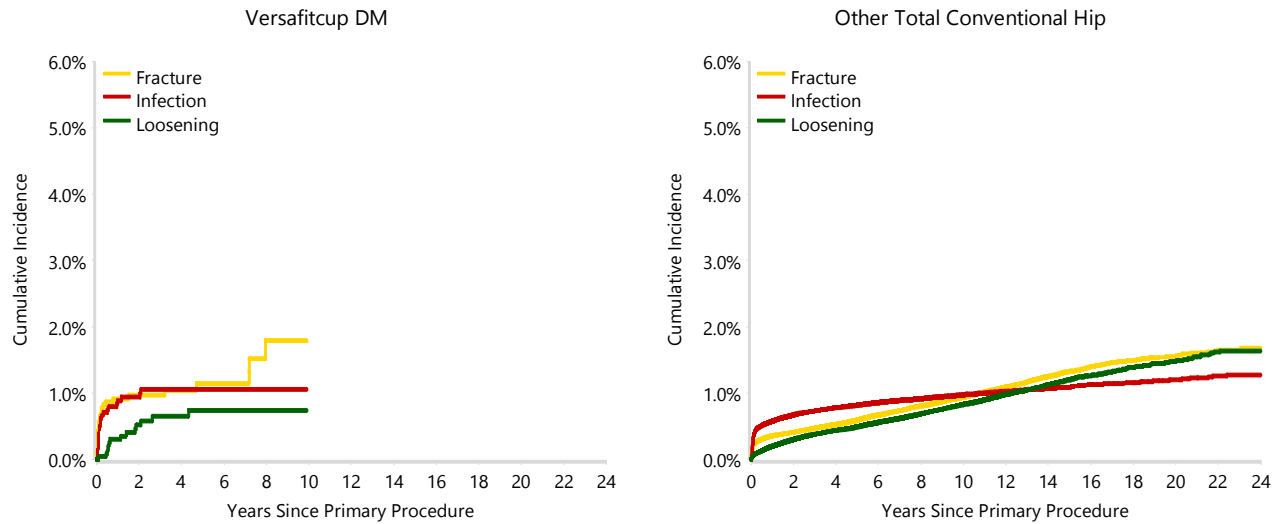


TABLE 5

Type of Revision Performed for Primary Total Conventional Hip Replacement

This analysis identifies the components used in the revision of the Versafitcup DM total conventional hip prosthesis and compares it to the components used in the revision of all other total conventional hip prostheses.

The reason this analysis is undertaken is to identify whether there is one or more components which are being replaced that differ from the components replaced for revisions of all other total conventional hip prostheses i.e. is there a difference in the type of revision undertaken for the Versafitcup DM total conventional hip prosthesis compared to all other total conventional hip prostheses.

Table 5: Primary Total Conventional Hip Replacement - Type of Revision (Follow-up Limited to 13.6 Years)

Type of Revision	Versafitcup DM		Other Total Conventional Hip	
	Number	Percent	Number	Percent
Femoral Component	34	41.0	6280	33.6
Acetabular Component	12	14.5	3214	17.2
THR (Femoral/Acetabular)	16	19.3	2092	11.2
Cement Spacer	2	2.4	584	3.1
Removal of Prostheses			95	0.5
Reinsertion of Components			29	0.2
Total Femoral			11	0.1
Bipolar Head and Femoral			9	0.0
N Major	64	77.1	12314	66.0
Head/Insert	17	20.5	4975	26.6
Head Only			911	4.9
Minor Components	1	1.2	293	1.6
Insert Only	1	1.2	175	0.9
Bipolar Only			1	0.0
Cement Only			1	0.0
Head/Neck			1	0.0
N Minor	19	22.9	6357	34.0
TOTAL	83	100.0	18671	100.0

Note: This table is restricted to revisions within 13.6 years for all groups to allow a time-matched comparison of revisions.

Note: Prostheses no longer used in 2024 are excluded from the comparator. Procedures using metal/metal prostheses with head size larger than 32mm are excluded from the comparator.

TABLE 6**Revision Rates of Versafitcup DM Primary Total Conventional Hip Replacement by Fixation**

This analysis is provided as some prostheses have more than one fixation option. Additionally there are prostheses where an alternative to the recommended approach to fixation was used e.g. a cementless prosthesis that has been cemented or vice-versa.

Table 6: Revised Number of Versafitcup DM Primary Total Conventional Hip Replacement by Fixation

Fixation	N Revised	N Total
Cemented	0	2
Cementless	73	1919
Hybrid (Femur Cemented)	10	526
TOTAL	83	2447

TABLE 7**Revision Rates of Versafitcup DM Primary Total Conventional Hip Replacement by Bearing Surface**

This analysis is provided as some prostheses are combined with a variety of bearing surfaces. All bearing surfaces used with this prosthesis are listed.

Table 7: Revised Number of Versafitcup DM Primary Total Conventional Hip Replacement by Bearing Surface

Bearing Surface	N Revised	N Total
Ceramic/Non XLPE	75	2114
Metal/Non XLPE	8	332
Ceramicised Metal/Non XLPE	0	1
TOTAL	83	2447

TABLE 8

Revision Rates of Versafitcup DM Primary Total Conventional Hip Replacement by Approach

This analysis is provided as some prostheses are used with a variety of surgical approaches. All surgical approaches used with this prosthesis are listed.

Table 8: Revised Number of Versafitcup DM Primary Total Conventional Hip Replacement by Approach

Approach	N Revised	N Total
Anterior	49	1514
Lateral	1	63
Posterior	31	812
TOTAL	81	2389

Note: Excludes 58 procedures with no approach recorded

TABLE 9**Number of Revisions of Versafitcup DM Primary Total Conventional Hip Replacement by Year of Implant**

This analysis details the number of prostheses reported each year to the Registry for the Versafitcup DM total conventional hip prosthesis. It also provides the subsequent number of revisions of the primaries reported in that year.

Primary procedures performed in later years have had less follow up time therefore the number revised is expected to be less than the number revised in earlier years. For example, a primary procedure performed in 2024 has a maximum of one year to be revised, whereas a primary procedure performed in 2022 has a maximum of three years to be revised.

Table 9: Number of Revisions of Versafitcup DM Primary Total Conventional Hip Replacement by Year of Implant

Year of Implant	Number Revised	Total Number
2011	0	10
2012	0	12
2013	0	4
2014	1	19
2015	11	146
2016	13	193
2017	13	199
2018	10	194
2019	10	188
2020	4	229
2021	3	249
2022	3	271
2023	9	381
2024	6	352
TOTAL	83	2447

TABLE 10

Revision Rates of Versafitcup DM Primary Total Conventional Hip Replacement by Component

A prosthesis may be combined with multiple components. This analysis has been undertaken to determine if the revision rate varies according to the component with which it is combined.

Table 10: Revised Number of Versafitcup DM Primary Total Conventional Hip Replacement by Femoral Stem Component

Femoral Stem Component	N Revised	N Total
AMiStem C	1	47
AMiStem H	7	250
AMiStem-P	0	6
CORAIL	0	6
CPCS	0	9
CPT	0	1
Collo-MIS	1	1
Cone	0	4
Exeter V40	0	1
GHE	3	14
LPS	0	2
M/L Taper	0	4
MasterLoc	3	131
MiniMax	5	125
Mistral	0	1
Modulus	0	1
Mutars	0	1
Polarstem	0	4
Quadra-C	8	405
Quadra-H	53	1293
Quadra-P	0	53
Quadra-R	1	3
Redapt	0	1
Revision Hip	0	7
S-Rom	0	2
Taperloc	0	19
Wagner	0	5
X-Acta	1	51
TOTAL	83	2447